




Steri-Tamp® Syringe & Container Instructions

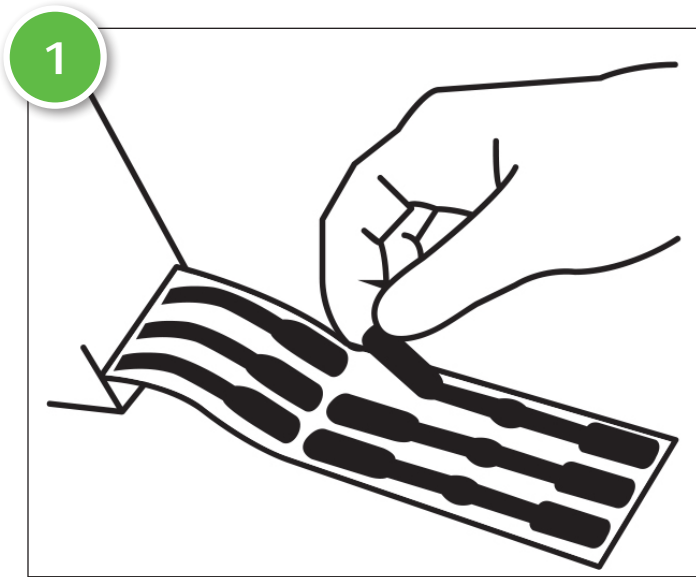


Remove Steri-Tamp® from liner.

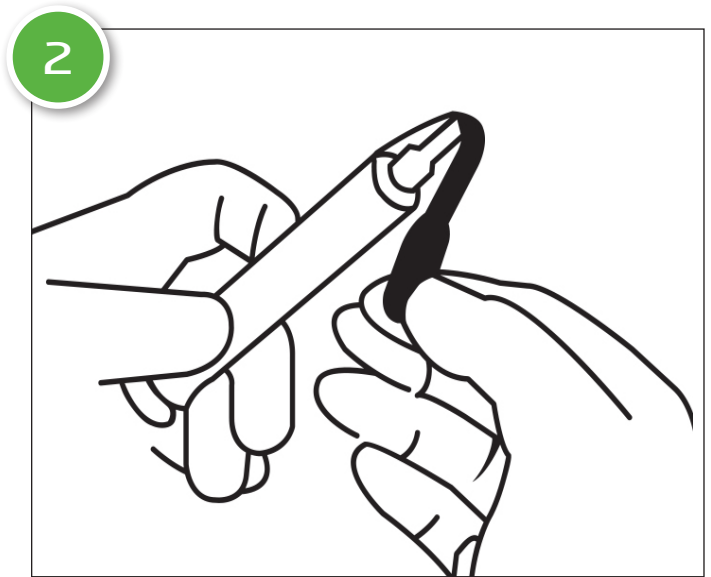

Position ends of Steri-Tamp® over syringe with the center covering the syringe cap.

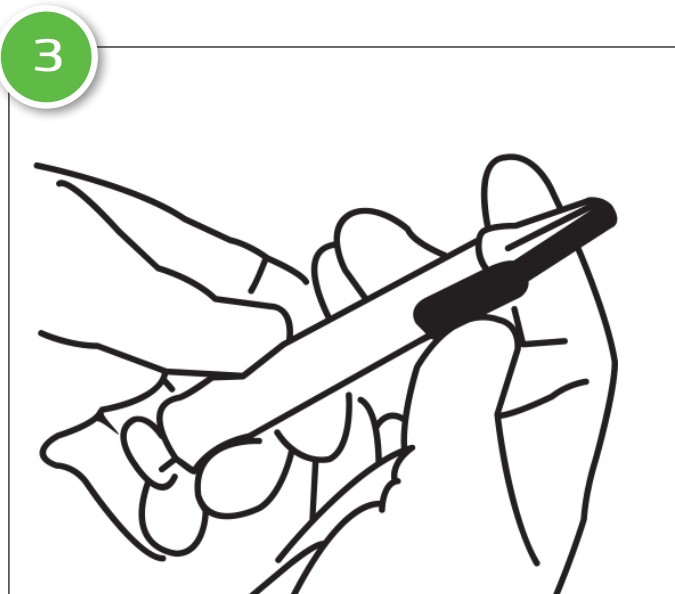

Press ends firmly to affix.

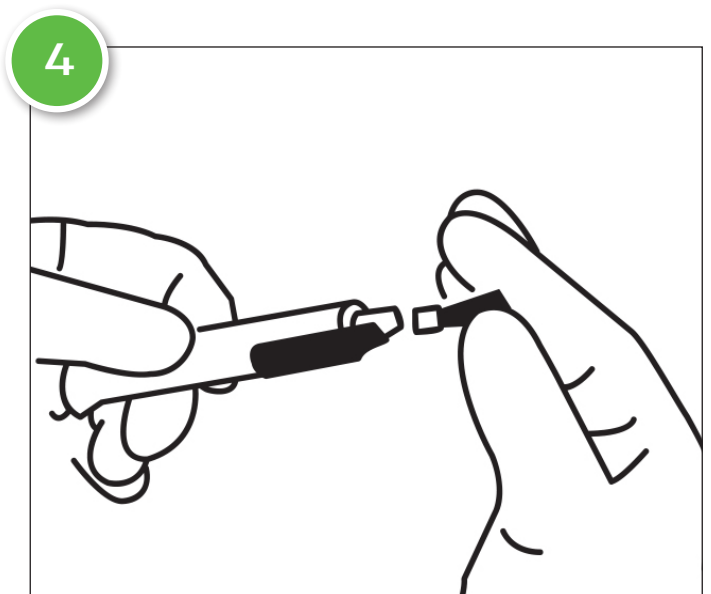

Upon removing the syringe cap, Steri-Tamp® will tear.

Steri-Tamp® may provide assistance in monitoring whether injectable products have already been used by indicating "OPENED" when the metalized layer is removed. Steri-Tamp® cannot be a substitute for good hospital practice and procedures.

NON-STERILE